

# Quantibody<sup>®</sup> Human Cell Adhesion Molecule Array 1

Quantitative measurement of 17 human cell adhesion molecules

Catalog #: QAH-CAM-1

User Manual  
Last revised July 18, 2019

Caution:  
Extraordinarily useful information enclosed



ISO 13485 Certified

3607 Parkway Lane, Suite 100  
Norcross, GA 30092

Tel: 1-888-494-8555 (Toll Free) or 770-729-2992, Fax: 770-206-2393  
Web: [www.RayBiotech.com](http://www.RayBiotech.com), Email: [info@raybiotech.com](mailto:info@raybiotech.com)

# Table of Contents

Section		Page #
I.	Overview	3
II.	Introduction	3
III.	How It Works	5
IV.	Materials Provided	6
V.	Storage	6
VI.	Additional Materials Required	6
VII.	General Considerations	7
	A. Sample Preparation	7
	B. Handling Glass Slides	7
	C. Incubation	7
VIII.	Protocol	8
	A. Completely Air Dry The Glass Slide	8
	B. Prepare Cytokine Standard Dilutions	8
	C. Blocking & Incubation	9
	D. Incubation with Biotinylated Antibody Cocktail & Wash	10
	E. Incubation with Cy3 Equivalent Dye-Streptavidin & Wash	10
	F. Fluorescence Detection	11
	G. Data Analysis	12
IX.	Array Map & Standard Curves	13
X.	Standard Concentrations	14
XI.	Spiking & Recovery	15
XII.	Q-Analyzer: Data Analysis Software	16
XIII.	Troubleshooting Guide	17
XIV.	Select Publications	18
XV.	Experiment Record Form	19
XVI.	How To Choose A Quantibody®	20

**Please read the entire manual carefully before starting your experiment**

## I. Overview

<b>Cytokines Detected (17)</b>	ALCAM (CD166), BCAM, CEACAM-1, E-Cadherin, TROP1 (EpCAM), E-Selectin, ICAM-1 (CD54), ICAM-2 (CD102), ICAM-3 (CD50), L-Selectin (CD62L), NCAM-1 (CD56), NrCAM, P-Cadherin, P-Selectin, PECAM-1 (CD31), VCAM-1 (CD106), VE-Cadherin (CDH5) <i>See Section IX for Array Map</i>
<b>Format</b>	One standard glass slide is spotted with 16 wells of identical cytokine antibody arrays. Each antibody is arrayed in quadruplicate.
<b>Detection Method</b>	Fluorescence. Go to <a href="http://www.RayBiotech.com/Scanners">www.RayBiotech.com/Scanners</a> for a list of compatible laser scanners.
<b>Sample Volume</b>	50 - 100 µl per array
<b>Reproducibility</b>	CV <20%
<b>Assay Duration</b>	6 hours

## II. Introduction

Cell Adhesion Molecules (CAMs) are transmembrane proteins located on the cell surface involved with the binding with other cells or with the extracellular matrix. CAMs mediate interactions between cells and their surroundings that are vital to processes controlling for cell proliferation, activation, migration, and survival. Based on their specific molecular structures, they are generally classified into four major CAM families: selectins, integrins, immunoglobulin (Ig)-like CAMs, and cadherins.

CAMs play an important role in many vital physiological processes. Altered levels of CAMs can be found in diverse diseases such as cardiovascular disease, stroke, cancer, Atherosclerosis, diabetes, and autoimmune disease. Recent advance showed increasing evidence that CAMs also play an important role in several neurological diseases, such as Alzheimer's disease, multiple sclerosis (MS) and Schizophrenia. Collective detection these molecules would help us to decipher their physiological functionality.

The traditional method for cytokine detection and quantification is through the use of an enzyme-linked immunosorbent assay (ELISA). In this method, target protein is immobilized to a solid support. The immobilized protein is then complexed with an antibody that is linked to an enzyme. Detection of the enzyme complex can then be visualized through the use of a substrate that produces a detectable signal. While this traditional method works well for a single protein, the overall procedure is time consuming and requires a relatively high volume of sample. Thus, conservation of precious small sample quantities

becomes a challenging task. Innovations in microarray technology over the last decade have addressed this problem. A long-standing leader in the field, Raybiotech, has pioneered the development of cytokine antibody arrays, which have now been widely applied in the research community with hundreds of peer reviewed publications, including top-tier journals such as *Cell* and *Nature*.

The Quantibody<sup>®</sup> array, our multiplexed sandwich ELISA-based quantitative array platform, enables researchers to accurately determine the concentration of multiple cytokines simultaneously. It combines the advantages of the high detection sensitivity & specificity of ELISA and the high throughput of arrays. Like a traditional sandwich-based ELISA, it uses a pair of cytokine specific antibodies for detection. A capture antibody is first bound to the glass surface. After incubation with the sample, the target cytokine is trapped on the solid surface. A second biotin-labeled detection antibody is then added, which can recognize a different epitope of the target cytokine. The cytokine-antibody-biotin complex can then be visualized through the addition of the streptavidin-conjugated Cy3 equivalent dye, using a laser scanner. Unlike the traditional ELISA, Quantibody products use an array format. By arraying multiple cytokine specific capture antibodies onto a glass support, quantitative, multiplex detection of cytokines in one experiment is made possible.

In detail, one standard glass slide is divided into 16 wells of identical cytokine antibody arrays. Each antibody, together with the positive controls is arrayed in quadruplicate. The slide comes with a 16-well removable gasket which allows for the process of 16 samples on one slide. Four slides can be nested into a tray, which matches a standard microplate footprint and allows for automated robotic high throughput process of 64 arrays simultaneously. For cytokine quantification, the array specific cytokine standards, whose concentration has been predetermined, are provided to generate a standard curve for each cytokine. In a real experiment, standard cytokines and samples will be assayed in each array simultaneously through a sandwich ELISA procedure. By comparing signals from unknown samples to the standard curve, the cytokine concentration in the samples will be determined.

Quantibody<sup>®</sup> array kits have been confirmed to have similar detection sensitivity as traditional ELISA. Our current high density Quantibody kits allow scientists to quantitatively determine the concentration of 1000 human, 200 mouse, and 67 rat cytokines in a single experiment. This is not only one of the most efficient products on the market for cytokine quantification, but makes it more affordable for quantification of large number of proteins. Simultaneous detection of multiple cytokines undoubtedly provides a powerful tool for drug and biomarker discovery.

### III. How It Works

---



## IV. Materials Provided

	Catalog #	Component Name	1 Slide Box	2 Slide Box*
1	QAH-CAM-1 S	Human Cell Adhesion Molecule Array 1 Glass Slide	1	2
2	QA-SDB	Quantibody <sup>®</sup> Sample Diluent	15 ml	
3	AA-WB1-30ML	20X Wash Buffer I	2 x 30 ml	3 x 30 ml
4	AA-WB2-30ML	20X Wash Buffer II	30 ml	
5	QAH-CAM-1 -STD	Human Cell Adhesion Molecule Array 1 Lyophilized Standard Mix**	1 Vial	
6	QAH-CAM-1 B	Human Cell Adhesion Molecule Array 1 Biotinylated Antibody Cocktail	1-25 µl	2 x 1-25 µl
7	QA-CY3E	Cy3 equivalent dye-conjugated Streptavidin	5 µl	2 x 5 µl
8	QA-SWD	Slide Washer/Dryer	1 x 30 ml Tube	
9	QA-ADH	Adhesive Film	1	2

\* 4 slide kits are comprised of 2 separate 2 slide kits.

\*\* See Section X for detailed cytokine concentrations after reconstitution.

## V. Storage

Upon receipt, all components should be stored at -20°C. The kit will retain activity for up to 6 months. Once thawed, the glass slide, standard mix, antibody cocktail and dye-conjugated Streptavidin should be kept at -20°C. All other components may be stored at 4°C. The entire kit should be used within 6 months of purchase.

## VI. Additional Materials Required

- Benchtop rocker or orbital rocker
- Laser scanner for fluorescence detection
- Aluminum foil
- Distilled water
- 1.5 ml Polypropylene microcentrifuge tubes

## VII. General Considerations

---

### A. Preparation of Samples

- Use serum-free conditioned media if possible.
- If serum-containing conditioned media is required, it is highly recommended that complete medium be used as a control since many types of sera contains cytokines.
- Each array needs 100  $\mu$ l of total sample volume. To avoid matrix effects, we recommend using a minimum of 2-fold sample dilution of culture media, body fluids, or 0.5-1mg/ml total protein for lysates, after a 5-fold to 10-fold dilution to minimize the effects of any detergent(s). Please be aware, more sample volume is required for combination arrays. For example, the minimum sample volume for a 10-array kit is 500  $\mu$ l, or 500  $\mu$ g lysate.
- The suggested serum/plasma dilution for this array is: 2x

### B. Handling Glass Slides

- Do not touch the surface of the slides, as the microarray slides are very sensitive. Hold the slides by the edges only.
- Handle all buffers and slides with powder free gloves.
- Handle glass slide/s in clean environment.
- Permanent marker ink can significantly interfere with fluorescent signal detection. To help distinguish one slide from another, you may make a small marking (such as a number or a star) along the top or bottom edge, using a green or blue ultra-fine point Sharpie<sup>®</sup> brand marker. This can also serve to orient the slide. For best results during scanning, please **DO NOT**:
  - Write anywhere on the front (arrayed) side of the slide
  - Write on the slide while it is wet
  - Use red or black colored ink anywhere on the slide
  - Write over the arrayed well areas of the slide, as this interferes with scanning.

### C. Incubation

- Completely cover array area with sample or buffer during incubation.
- Avoid foaming during incubation steps.
- Perform all incubation and wash steps under gentle rocking or rotation.
- Cover the incubation chamber with adhesive film during incubation, particularly when incubation is more than 2 hours or <70  $\mu$ l of sample or reagent is used.

- Several incubation steps such as step 6 (blocking), step 7 (sample incubation), step 10 (detection antibody incubation), or step 13 (Cy3 equivalent dye-streptavidin incubation) may be done overnight at 4°C. Please make sure to cover the incubation chamber tightly to prevent evaporation.

## VIII. Protocol

---

### A. Completely Air Dry The Glass Slide

1. Take out the glass slide from the box, and let it equilibrate to room temperature inside the sealed plastic bag for 20-30 minutes. Remove slide from the plastic bag, peel off the cover film, and let it air dry for another 1-2 hours.

*Incomplete drying of slides before use may cause the formation of "comet tails," thin directional smearing of antibody spots.*

### B. Prepare Cytokine Standard Dilutions

*There is only one vial of standard provided in the two-slide kit, which is enough for making two standard curves. Reconstitute the lyophilized standard within one hour of usage. If you must use the standard for two different days, store only the Std1 dilution at -80°C.*



2. Reconstitute the Cytokine Standard Mix (lyophilized) by adding 500 µl Sample Diluent to the tube. For best recovery, always quick-spin vial prior to opening. Dissolve the powder thoroughly by a gentle mix. Labeled the tube as Std1.



3. Label 6 clean microcentrifuge tubes as Std2 to Std7. Add 200  $\mu$ l Sample Diluent to each of the tubes.
4. Pipette 100  $\mu$ l Std1 into tube Std2 and mix gently. Perform 5 more serial dilutions by adding 100  $\mu$ l Std2 to tube Std3 and so on.
5. Add 100  $\mu$ l Sample Diluent to another tube labeled as CNTRL. Do not add standard cytokines or samples to the CNTRL tube, which will be used as negative control. For best results, include a set of standards in each slide.

*Since the starting concentration of each cytokine is different, the serial concentrations from Std1 to Std7 for each cytokine are varied which can be found in Section X.*

### **C. Blocking & Incubation**

6. Add 100  $\mu$ l Sample Diluent into each well and incubate at room temperature for 30 minutes to block slides.
7. Decant buffer from each well. Add 100  $\mu$ l standard cytokines or samples to each well. Incubate arrays at room temperature for 1-2 hour.

*Longer incubation time is preferable for higher signals. This step may be done overnight at 4°C.*

*We recommend using 50 to 100  $\mu$ l of original or diluted serum, plasma, conditioned media, or other body fluid, or 250  $\mu$ g/ml-1 mg/ml of protein for cell and tissue lysates. Cover the incubation chamber with adhesive film during incubation, especially if less than 70  $\mu$ l of sample or reagent is used.*

#### 8. Wash:

- Decant the samples from each well, and wash 5 times (5 min each) with 150  $\mu$ l of 1X Wash Buffer I at room temperature with gentle rocking. Completely remove wash buffer in each wash step. Dilute 20x Wash Buffer I with H<sub>2</sub>O.
- *(Optional for Cell and Tissue Lysates)* Put the glass slide with frame into a box with 1X Wash Buffer I (cover the whole glass slide and frame with Wash Buffer

l), and wash at room temperature with gentle rocking for 20 min.

- Decant the 1x Wash Buffer I from each well, wash 2 times (5 min each) with 150  $\mu$ l of 1X Wash Buffer II at room temperature with gentle rocking. Completely remove wash buffer in each wash step. Dilute 20X Wash Buffer II with H<sub>2</sub>O.

*Incomplete removal of the wash buffer in each wash step may cause "dark spots," the background signals higher than the spots.*

#### **D. Incubation with Biotinylated Antibody Cocktail & Wash**

9. Reconstitute the detection antibody by adding 1.4 ml of Sample Diluent to the tube. Spin briefly.
10. Add 80  $\mu$ l of the detection antibody cocktail to each well. Incubate at room temperature for 1-2 hour.

*Longer incubation time is preferable for higher signals and backgrounds*


11. Decant the samples from each well, and wash 5 times (5 mins each) with 150  $\mu$ l of 1X Wash Buffer I and then 2 times with 150  $\mu$ l of 1x Wash Buffer II at room temperature with gentle rocking. Completely remove wash buffer in each wash step.

#### **E. Incubation with Cy3 Equivalent Dye-Streptavidin & Wash**

12. After briefly spinning down, add 1.4 ml of Sample Diluent to Cy3 equivalent dye-conjugated streptavidin tube. Mix gently.
13. Add 80  $\mu$ l of Cy3 equivalent dye-conjugated streptavidin to each well. Cover the device with aluminum foil to avoid exposure to light or incubate in dark room. Incubate at room temperature for 1 hour.  
Decant the samples from each well, and wash 5 times (5 mins each) with 150  $\mu$ l of 1X Wash Buffer I at room temperature with gentle rocking. Completely remove wash buffer in each wash step.
14.  $\mu$ l of 1X Wash Buffer I at room temperature with gentle rocking. Completely remove wash buffer in each wash step.

## F. Fluorescence Detection

15. Disassemble the device by pushing clips outward from the slide side. Carefully remove the slide from the gasket.

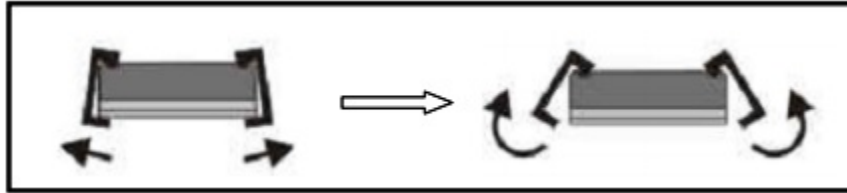

*Be careful not to touch the surface of the array side.*

16. Place the slide in the Slide Washer/Dryer (a 4-slide holder/centrifuge tube), add enough 1x Wash Buffer I (about 30 ml) to cover the whole slide, and then gently shake at room temperature for 15 minutes. Decant Wash Buffer I. Wash with 1x Wash Buffer II (about 30 ml) and gently shake at room temperature for 5 minutes.
17. Remove water droplets completely by gently applying suction with a pipette to remove water droplets. Do not touch the array, only the sides.

*You may also dry the glass slide by a compressed N<sub>2</sub> stream.*


18. Imaging: The signals can be visualized through use of a laser scanner equipped with a Cy3 wavelength (green channel) such as Axon GenePix or Innopsys Innoscan. Make sure that the signal from the well containing the highest standard concentration (Std1) receives the highest possible reading, yet remains unsaturated.

*In case the signal intensity for different cytokine varies greatly in the same array, we recommend using multiple scans, with a higher PMT for low signal cytokines, and a low PMT for high signal cytokines.*

## G. Data Analysis

19. Data extraction can be done using the GAL file that is specific for this array along with the microarray analysis software (GenePix, ScanArray Express, ArrayVision, MicroVigene, etc.). GAL files can be found here: [www.RayBiotech.com/Gal-Files.html](http://www.RayBiotech.com/Gal-Files.html).


Need help analyzing all that data? Copy and paste your data into the Q-Analyzer Tool specific for this array, catalog number: **QAH-CAM-1-SW**. More information can be found in Section XII.

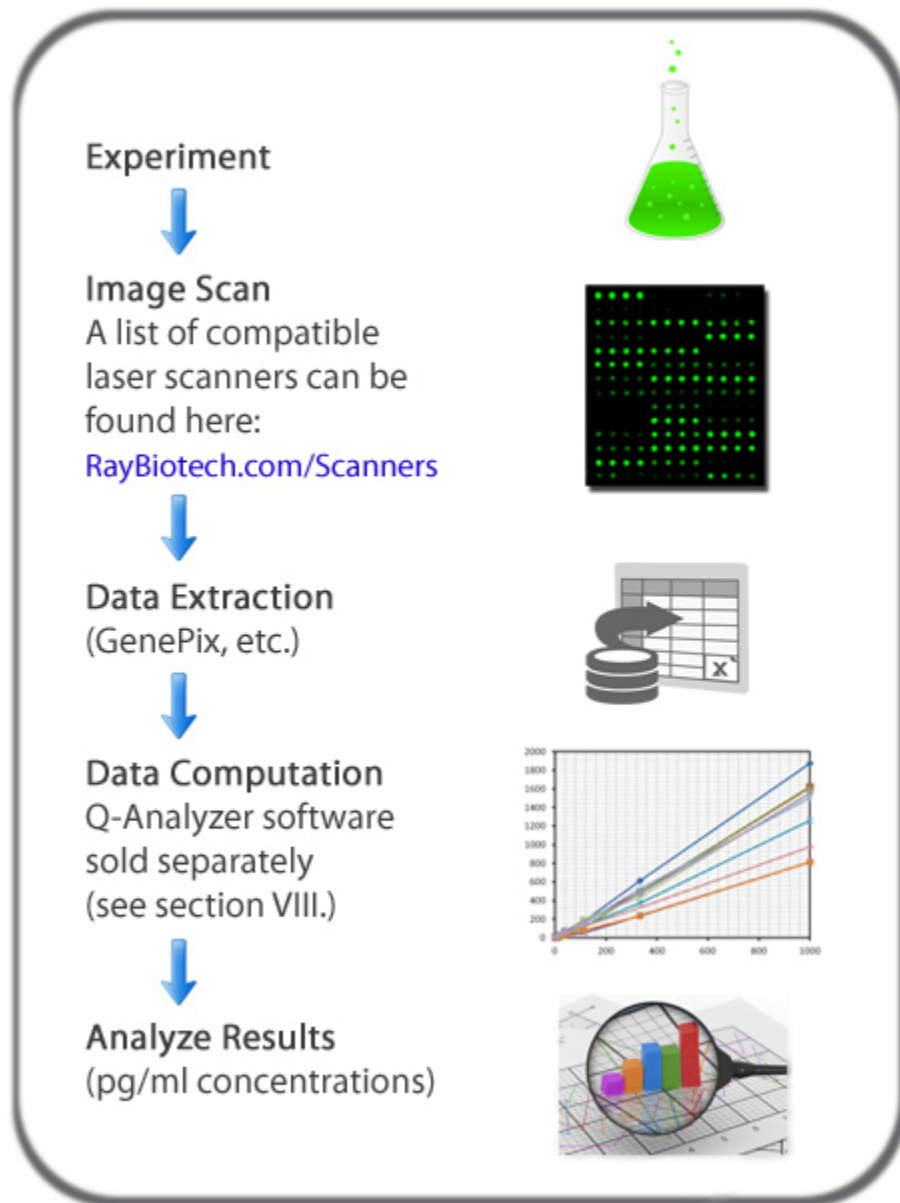

## IX. Array Map & Standard Curves

Each antibody is printed in quadruplicate horizontally									
	1	2	3	4	1	2	3	4	
A	POS1				POS2				
B	ALCAM (CD166)				BCAM				
C	CEACAM-1				E-Cadherin				
D	TROP1 (EpCAM)				E-Selectin				
E	ICAM-1 (CD54)				ICAM-2 (CD102)				
F	ICAM-3 (CD50)				L-Selectin (CD62L)				
G	NCAM-1 (CD56)				NrCAM				
H	P-Cadherin				PECAM-1 (CD31)				
I	P-Selectin				VCAM-1 (CD106)				
J	VE-Cadherin (CDH5)				NEG				

### QAH-CAM-1 Standard Curves

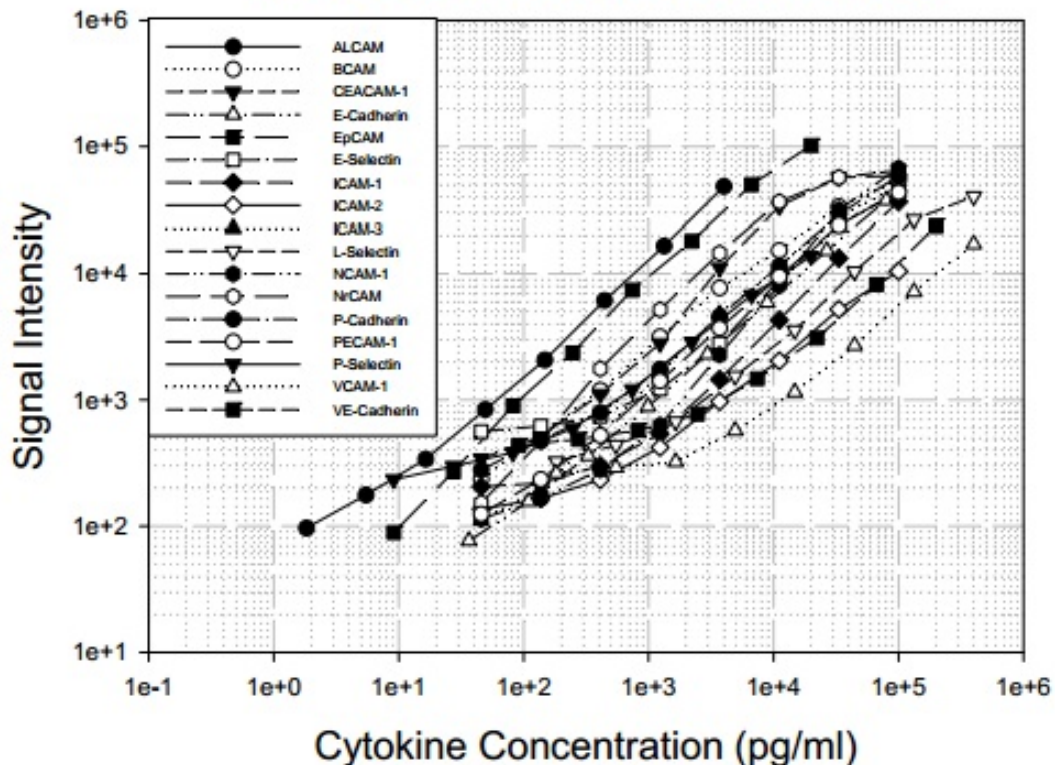



## X. Standard Concentrations

---

After reconstitution, the lyophilized cytokine standard mix contains the following concentrations for each antigen included.

*Serial standard concentration (pg/ml)*

(pg/ml)	Control	Std7	Std6	Std5	Std4	Std3	Std2	Std1
ALCAM	0	5	16	49	148	444	1,333	4,000
BCAM	0	137	412	1,235	3,704	11,111	33,333	100,000
CEACAM-1	0	137	412	1,235	3,704	11,111	33,333	100,000
E-Cadherin	0	110	329	988	2,963	8,889	26,667	80,000
EpCAM	0	27	82	247	741	2,222	6,667	20,000
E-Selectin	0	137	412	1,235	3,704	11,111	33,333	100,000
ICAM-1	0	137	412	1,235	3,704	11,111	33,333	100,000
ICAM-2	0	137	412	1,235	3,704	11,111	33,333	100,000
ICAM-3	0	137	412	1,235	3,704	11,111	33,333	100,000
L-Selectin	0	549	1,646	4,938	14,815	44,444	133,333	400,000
NCAM-1	0	137	412	1,235	3,704	11,111	33,333	100,000
NrCAM	0	137	412	1,235	3,704	11,111	33,333	100,000
P-Cadherin	0	137	412	1,235	3,704	11,111	33,333	100,000
PECAM-1	0	137	412	1,235	3,704	11,111	33,333	100,000
P-Selectin	0	27	82	247	741	2,222	6,667	20,000
VCAM-1	0	549	1,646	4,938	14,815	44,444	133,333	400,000
VE-Cadherin	0	274	823	2,469	7,407	22,222	66,667	200,000

## **XI. Spiking & Recovery**

---

The antibody pairs used in the kit have been tested to recognize their specific antigen. The spiking recovery rates of each protein in some common fluids are listed in the following tables.

### *System cross-reactivity test*

CAB/DAB	ALCAM	BCAM	CEACAM-1	E-Cadherin	EpCAM	E-Selectin	ICAM-1	ICAM-2	ICAM-3	L-Selectin	NCAM-1	NrCAM	P-Cadherin	PECAM-1	P-selectin	VCAM-1	VE-Cadherin
ALCAM	29114	17	13	387	28	18	21	24	13	9	36	68	36	18	10	4	17
BCAM	70	9727	63	230	58	67	80	105	88	81	73	436	123	75	38	61	78
CEACAM-1	12	36	11582	62	18	30	6	26	29	36	16	121	34	40	24	29	42
E-Cadherin	23	231	30	14900	29	30	14	75	38	45	21	86	184	33	14	24	47
EpCAM	17	1	15	256	27806	6	15	16	1	9	15	29	20	15	1	1	27
E-Selectin	72	79	70	171	71	6535	69	95	58	70	69	313	91	57	47	59	79
ICAM-1	23	18	18	33	116	15	11157	12	6	18	7	53	26	12	6	9	16
ICAM-2	43	33	50	212	54	58	34	14699	54	42	31	54	72	40	18	23	64
ICAM-3	28	16	19	67	36	5	32	12	14331	26	9	14	28	12	17	5	20
L-Selectin	47	73	68	117	69	63	49	113	44	9511	38	238	95	68	14	41	68
NCAM-1	44	18	47	19	65	38	41	44	41	64	47151	39	49	38	27	63	48
NrCAM	25	12	31	106	18	34	17	27	8	8	24	13317	38	27	8	41	36
P-Cadherin	41	13	28	290	21	41	25	15	7	18	31	131	27786	33	1	18	54
PECAM-1	19	1	8	14	4	18	4	20	9	3	4	26	17	6285	1	6	1
P-selectin	169	74	99	72	105	125	94	110	136	101	84	54	126	56	41235	104	155
VCAM-1	57	44	78	79	102	78	53	85	91	38	48	100	151	77	31	8943	78
VE-Cadherin	158	30	63	448	58	66	46	55	43	53	30	228	94	50	28	58	21749

### *The spiking recovery rate for culture media and serum*

(pg/ml)	Spiking	CM	CM+Ag	CM%	Serum	Serum+Ag	Serum%
ALCAM	2,000	0	1,973	99%	41	1,886	92%
BCAM	50,000	0	43,543	87%	0	30,477	61%
CEACAM-1	50,000	0	48,175	96%	394	30,163	60%
E-Cadherin	40,000	0	12,708	32%	0	12,480	31%
EpCAM	10,000	0	9,137	91%	0	6,274	63%
E-Selectin	50,000	0	57,754	116%	307	38,574	77%
ICAM-1	50,000	0	41,004	82%	54,633	112,939	117%
ICAM-2	50,000	0	27,273	55%	14,330	32,617	37%
ICAM-3	50,000	0	31,862	64%	0	31,518	63%
L-Selectin	200,000	0	137,506	69%	73,849	196,903	62%
NCAM-1	50,000	2,184	65,343	126%	24,689	79,904	110%
NrCAM	50,000	0	45,917	92%	0	30,221	60%
P-Cadherin	50,000	630	47,044	93%	3,716	62,841	118%
PECAM-1	50,000	0	38,203	76%	0	37,333	75%
P-selectin	10,000	0	11,348	113%	2,029	13,415	114%
VCAM-1	200,000	0	228,073	114%	10,674	133,383	61%
VE-Cadherin	100,000	0	38,297	38%	0	40,056	40%



## XII. Quantibody<sup>®</sup> Q-Analyzer

---

The Q-Analyzer is an array specific, Excel-based program. It is much more than a simple calculation macro; it performs sophisticated data analysis (see below for description).

The Q-Analyzer Tool specific for this array is catalog number: **QAH-CAM-1-SW**.

### Key features:

- Simplicity: Easy to operate and requires no professional training. With a simple copy and paste process, the cytokine concentration is determined.
- Outlier Marking & Removing: The software can automatically mark and remove the outlier spots for more accurate data analysis
- Normalization: The program allows for intra- and inter-slide normalization for large numbers of samples.
- Two Positive Controls: The program utilizes the two positive controls in each array for normalization.
- Two Analytical Algorithms: Users can choose either linear regression or log-log algorithms to meet their analytical needs.
- Two Data Outputs: standard curves and digital concentration.
- User Intervention: The program allows for user manual handling of outliers and other analytical data.
- Lower and Upper Limits Determination: The program automatically marks out the values below or above the detection range.
- Standard Deviation: The program outputs the standard deviations of the quadruplicate spots for data accuracy.
- Analytical Tips: Q-Analyzer analysis tips are included in the program.

### XIII. Troubleshooting Guide

<b>Problem</b>	<b>Cause</b>	<b>Recommendation</b>
<b>Weak Signal</b>	Inadequate detection	Increase laser power and PMT parameters
	Inadequate reagent volumes or improper dilution	Check pipettes and ensure correct preparation
	Short incubation time	Increase incubation time or change sample incubation step to overnight
	Too low protein concentration in sample	Lessen dilution or do not dilute sample. Concentrate sample if necessary.
	Improper storage of kit	Store kit as suggested temperature. Don't freeze/thaw the slide.
<b>Uneven signal</b>	Bubble formed during incubation	Decrease amount of rocking during incubations. check for bubble formation and remove bubbles.
	Arrays are not completely covered by reagent	Completely cover arrays with solution for all required steps.
	Reagent evaporation	Cover the incubation chamber with adhesive film during incubation
<b>Poor standard curve</b>	Cross-contamination from neighboring wells	Avoid overflowing wash buffer and other solutions into neighboring wells.
	Comet tail formation	Air dry the slide for at least 1 hour before usage
	Inadequate standard reconstitution or Improper dilution	Reconstitute the lyophilized standard well at the room temperature before making serial dilutions. Check pipettes and ensure proper serial dilutions.
	Inadequate detection	Increase laser power so the highest standard concentration for each cytokine receives the highest possible reading yet remains unsaturated.
	Use freeze-thawed cytokine standards	Always use new cytokine standard vial for new set of experiment. Discard any leftover.
<b>High background</b>	Overexposure	Lower the PMT or signal gain.
	Dark spots	Completely remove wash buffer in each wash step.
	Insufficient wash	Increase wash time and use more wash buffer
	Dust	Work in clean environment
	Slide is allowed to dry out	Don't dry out slides during experiment.

## XIV. Select Quantibody<sup>®</sup> Publications

---

1. Zeng Q., et al. The functional behavior of a macrophage/fibroblast co-culture model derived from normal and diabetic mice with a marine gelatin-oxidized alginate hydrogel. *Biomaterials*. 2010 Aug;31(22):5772-81. doi: 10.1016/j.biomaterials.2010.04.022.  
**Species:** Mouse
2. Toh H, Wang W, Chia W, Kvistborg P, Sun Li, et al. Clinical Benefit of Allogeneic Melanoma Cell Lysate-Pulsed Autologous Dendritic Cell Vaccine in MAGE-Positive Colorectal Cancer Patients. *Clin Cancer Res*. 2009;15(24):7726-7736  
**Species:** Human  
**Sample Type:** Plasma
3. Du Y, Wei X, He Y, Wei G, Hampel H, et al. P2-380: Identification and characterization of human autoantibodies that may be used for the treatment of prion diseases. *Alzheimer Dementia*. 2008;4(4 Suppl):T484 (Abstract P2-380).  
**Species:** Human  
**Sample Type:** Plasma
4. Jonnalagadda D., et al. Platelet secretion is kinetically heterogeneous in an agonist-responsive manner. December 20, 2012; *Blood*: 120 (26). <http://dx.doi.org/10.1182/blood-2012-07-445080>  
**Species:** Human  
**Sample Type:** Conditioned Media
5. Vargas-Inchaustegui D., Hogg A., Tulliano G., et al. CXCL10 Production by Human Monocytes in Response to *Leishmania braziliensis* Infection. *Infect. Immun*. January 2010 vol. 78 no. 1 301-308  
**Species:** Human  
**Sample Type:** Serum
6. Zhai Y, Zhong Z, Chen C-YA, Xia Z, Song L, Blackburn MR, Shyu A-B. Coordinated Changes in mRNA Turnover, Translation, and RNA Processing Bodies in Bronchial Epithelial Cells following Inflammatory Stimulation. *Mol Cell Biol*. 2008; 28(24):7414-7426.  
**Species:** Human
7. Huggenberger R., et al. Stimulation of lymphangiogenesis via VEGFR-3 inhibits chronic skin inflammation. *J Exp Med*. 2010 Sep 27;207(10):2255-69. doi: 10.1084/jem.20100559.  
**Species:** Mouse  
**Sample Type:** Tissue Lysate
8. Jurk D., Wilson C., Passos J., et al. Chronic inflammation induces telomere dysfunction and accelerates ageing in mice. *Nature Communications* 2, Article number: 4172. doi:10.1038/ncomms5172  
**Species:** Mouse  
**Sample Type:** Conditioned Media
9. Bethunaickan, R., Sahu, R., Liu, Z., Tang, Y. T., Huang, W., Edegbe, O., Tao, H., Ramanujam, M., Madaio, M. P. and Davidson, A. (2012), Anti-tumor necrosis factor alpha treatment of interferon-alpha-induced murine lupus nephritis reduces the renal macrophage response but does not alter glomerular immune complex formation. *Arthritis & Rheumatism*, 64: 3399-3408. doi: 10.1002/art.34553  
**Species:** Mouse  
**Sample Type:** Tissue Lysate
10. Hou T., Li Z., Luo F., Xie Z., Wu X., Xing J., Dong S., Xu J. A composite demineralized bone matrix e Self assembling peptide scaffold for enhancing cell and growth factor activity in bone marrow. *Biomaterials*, Available online 19 April 2014. [Epub ahead of print]  
**Species:** Mouse  
**Sample Type:** Tissue Lysate
11. Feng W., Madajka M., Kerr B., Mahabeleshwar G., White S., Byzova T. A novel role for platelet secretion in angiogenesis: mediating bone marrow-derived cell mobilization and homing. *Blood* April 7, 2011 vol. 117 no. 14 3893-3902  
**Species:** Mouse

# XV. Experiment Record Form

---


Date: \_\_\_\_\_

File Name: \_\_\_\_\_

Laser Power: \_\_\_\_\_

PMT: \_\_\_\_\_

Well No.	Sample Name	Dilution factor
1	CNTRL	
2	Std7	
3	Std6	
4	Std5	
5	Std4	
6	Std3	
7	Std2	
8	Std1	
9		
10		
11		
12		
13		
14		
15		
16		

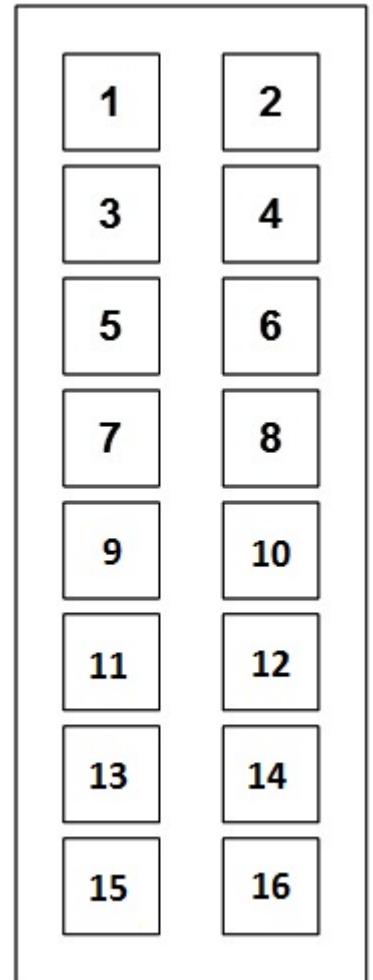

## XVI. How to Choose a Quantibody<sup>®</sup> Array?

### Species-based selection:

Human (QAH-)	Mouse (QAM-)	Rat (QAR-)	Bovine (QAB-)	Canine (QAC-)
Equine (QAE-)	Feline (QAF-)	Primates (QAN-)	Porcine (QAP-)	Rabbit (QAL-)

### Function-based selection:

Adhesion Molecule Arrays	Angiogenesis Arrays	Bone Metabolism Arrays	Chemokine Arrays
<b>Custom Arrays</b>	Cytokine Arrays	Growth Factor Arrays	IGF Signaling Arrays
IL-1 Family Arrays	Immune Response Arrays	Inflammation Arrays	Interleukin Arrays
Isotyping Arrays	MMP Arrays	Obesity Arrays	Ophthalmic Arrays
Periodontal Disease Arrays	Receptor Arrays	Th1/Th2/Th17 Arrays	

### Cytokine Number-based selection:

Arrays are available in the Quantibody<sup>®</sup> platform to detect 1000 human, 200 mouse, or 67 rat proteins. GLP-Compliant testing services are also available.

To learn more about the Quantibody<sup>®</sup> Antibody Array, visit [www.RayBiotech.com/Quantibody-Multiplex-Elisa-Array.html](http://www.RayBiotech.com/Quantibody-Multiplex-Elisa-Array.html)

Quantibody<sup>®</sup> is the trademark of RayBiotech, Inc.  
This product is for research use only.



©2019 RayBiotech, Inc