

# Quantibody<sup>®</sup> Mouse Cytokine Antibody Array 3000

A combination of 4 non-overlapping arrays to quantitatively measure  
160 mouse cytokines

Catalog #: QAM-CAA-3000

User Manual  
Last revised 5-Dec-18

Caution:  
Extraordinarily useful information enclosed



ISO 13485 Certified

3607 Parkway Lane, Suite 100  
Norcross, GA 30092

Tel: 1-888-494-8555 (Toll Free) or 770-729-2992, Fax: 770-206-2393  
Web: [www.RayBiotech.com](http://www.RayBiotech.com), Email: [info@raybiotech.com](mailto:info@raybiotech.com)

# Table of Contents

Section		Page #
I.	Overview	3
II.	Introduction	3
III.	How It Works	5
IV.	Materials Provided	6
V.	Storage	6
VI.	Additional Materials Required	6
VII.	General Considerations	7
	A. Sample Preparation	7
	B. Handling Glass Slides	7
	C. Incubation	7
VIII.	Protocol	8
	A. Completely Air Dry The Glass Slide	8
	B. Prepare Cytokine Standard Dilutions	8
	C. Blocking & Incubation	9
	D. Incubation with Biotinylated Antibody Cocktail & Wash	10
	E. Incubation with Cy3 Equivalent Dye-Streptavidin & Wash	10
	F. Fluorescence Detection	11
	G. Data Analysis	12
IX.	Array Map & Standard Curves	13
X.	Standard Concentrations	14
XI.	Spiking & Recovery	15
XII.	Q-Analyzer: Data Analysis Software	16
XIII.	Troubleshooting Guide	17
XIV.	Select Publications	18
XV.	Experiment Record Form	19
XVI.	How To Choose A Quantibody®	20

**Please read the entire manual carefully before starting your experiment**

## I. Overview

<b>Cytokines Detected (160)</b>	Arrays Included: QAM-CYT-4 (40); QAM-CYT-5 (40); QAM-CYT-6 (40); QAM-CY-7 (40) <i>See Section IX for Array Map</i>
<b>Format</b>	One standard glass slide is spotted with 16 wells of identical cytokine antibody arrays. Each antibody is arrayed in quadruplicate.
<b>Detection Method</b>	Fluorescence. Go to <a href="http://www.RayBiotech.com/Scanners">www.RayBiotech.com/Scanners</a> for a list of compatible laser scanners.
<b>Sample Volume</b>	50 - 100 µl per array
<b>Reproducibility</b>	CV <20%
<b>Assay Duration</b>	6 hours

## II. Introduction

Cytokines play an important role in innate immunity, apoptosis, angiogenesis, cell growth and differentiation. They are involved in interactions between different cell types, cellular responses to environmental conditions, and maintenance of homeostasis. In addition, cytokines are also involved in most disease processes, including cancer and cardiac diseases.

The traditional method for cytokine detection and quantification is through the use of an enzyme-linked immunosorbent assay (ELISA). In this method, target protein is immobilized to a solid support. The immobilized protein is then complexed with an antibody that is linked to an enzyme. Detection of the enzyme complex can then be visualized through the use of a substrate that produces a detectable signal. While this traditional method works well for a single protein, the overall procedure is time consuming and requires a relatively high volume of sample. Thus, conservation of precious small sample quantities becomes a challenging task. Innovations in microarray technology over the last decade have addressed this problem. A long-standing leader in the field, Raybiotech, has pioneered the development of cytokine antibody arrays, which have now been widely applied in the research community with hundreds of peer reviewed publications, including top-tier journals such as *Cell* and *Nature*.

The Quantibody<sup>®</sup> array, our multiplexed sandwich ELISA-based quantitative array platform, enables researchers to accurately determine the concentration of multiple cytokines simultaneously. It combines the advantages of the high detection sensitivity & specificity of ELISA and the high throughput of arrays. Like a traditional sandwich-based ELISA, it uses a pair of cytokine specific antibodies for detection. A capture antibody is first bound to the glass surface. After incubation with the sample, the target cytokine is

trapped on the solid surface. A second biotin-labeled detection antibody is then added, which can recognize a different epitope of the target cytokine. The cytokine-antibody-biotin complex can then be visualized through the addition of the streptavidin-conjugated Cy3 equivalent dye, using a laser scanner. Unlike the traditional ELISA, Quantibody products use an array format. By arraying multiple cytokine specific capture antibodies onto a glass support, quantitative, multiplex detection of cytokines in one experiment is made possible.

In detail, one standard glass slide is divided into 16 wells of identical cytokine antibody arrays. Each antibody, together with the positive controls is arrayed in quadruplicate. The slide comes with a 16-well removable gasket which allows for the process of 16 samples on one slide. Four slides can be nested into a tray, which matches a standard microplate footprint and allows for automated robotic high throughput process of 64 arrays simultaneously. For cytokine quantification, the array specific cytokine standards, whose concentration has been predetermined, are provided to generate a standard curve for each cytokine. In a real experiment, standard cytokines and samples will be assayed in each array simultaneously through a sandwich ELISA procedure. By comparing signals from unknown samples to the standard curve, the cytokine concentration in the samples will be determined.

Quantibody<sup>®</sup> array kits have been confirmed to have similar detection sensitivity as traditional ELISA. Our current high density Quantibody kits allow scientists to quantitatively determine the concentration of 1000 human, 200 mouse, and 67 rat cytokines in a single experiment. This is not only one of the most efficient products on the market for cytokine quantification, but makes it more affordable for quantification of large number of proteins. Simultaneous detection of multiple cytokines undoubtedly provides a powerful tool for drug and biomarker discovery.

### III. How It Works

---



## IV. Materials Provided

*This product is a combination of multiple arrays. Items 1, 5, & 6 are array-specific.*

	Catalog #	Component Name	1 Slide Box	2 Slide Box*
1	[Array-Cat-#]S	Array-specific Glass Slide	1	2
2	QA-SDB	Quantibody <sup>®</sup> Sample Diluent	15 ml	
3	AA-WB1-30ML	20X Wash Buffer I	2 x 30 ml	3 x 30 ml
4	AA-WB2-30ML	20X Wash Buffer II	30 ml	
5	[Array-Cat-#]-STD	Array-specific Lyophilized Standard Mix**	1 Vial	
6	[Array-Cat-#]B	Array-specific Biotinylated Antibody Cocktail	1-25 µl	2 x 1-25 µl
7	QA-CY3E	Cy3 equivalent dye-conjugated Streptavidin	5 µl	2 x 5 µl
8	QA-SWD	Slide Washer/Dryer	1 x 30 ml Tube	
9	QA-ADH	Adhesive Film	1	2

\* 4 slide kits are comprised of 2 separate 2 slide kits.

\*\* See Section X for detailed cytokine concentrations after reconstitution.

## V. Storage

Upon receipt, all components should be stored at -20°C. The kit will retain activity for up to 6 months. Once thawed, the glass slide, standard mix, antibody cocktail and dye-conjugated Streptavidin should be kept at -20°C. All other components may be stored at 4°C. The entire kit should be used within 6 months of purchase.

## VI. Additional Materials Required

- Benchtop rocker or orbital rocker
- Laser scanner for fluorescence detection
- Aluminum foil
- Distilled water
- 1.5 ml Polypropylene microcentrifuge tubes

## VII. General Considerations

---

### A. Preparation of Samples

- Use serum-free conditioned media if possible.
- If serum-containing conditioned media is required, it is highly recommended that complete medium be used as a control since many types of sera contains cytokines.
- Each array needs 100  $\mu$ l of total sample volume. To avoid matrix effects, we recommend using a minimum of 2x dilution for serum, plasma, cell culture media, or other body fluids, or 500  $\mu$ g/ml-1 mg/ml (after a 5-fold to 10-fold dilution to minimize the effects of any detergent(s)) total protein for cell and tissue lysates. Please be aware, more sample volume is required for combination arrays. For example, the minimum sample volume for a 10-array kit is 500  $\mu$ l, or 500  $\mu$ g cell lysate.

*If you experience high background or if the fluorescent signal intensities exceed the detection range, further dilution of your sample is recommended.*

### B. Handling Glass Slides

- Do not touch the surface of the slides, as the microarray slides are very sensitive. Hold the slides by the edges only.
- Handle all buffers and slides with powder free gloves.
- Handle glass slide/s in clean environment.
- Permanent marker ink can significantly interfere with fluorescent signal detection. To help distinguish one slide from another, you may make a small marking (such as a number or a star) along the top or bottom edge, using a green or blue ultra-fine point Sharpie<sup>®</sup> brand marker. This can also serve to orient the slide. For best results during scanning, please **DO NOT**:
  - Write anywhere on the front (arrayed) side of the slide
  - Write on the slide while it is wet
  - Use red or black colored ink anywhere on the slide
  - Write over the arrayed well areas of the slide, as this interferes with scanning.

### C. Incubation

- Completely cover array area with sample or buffer during incubation.
- Avoid foaming during incubation steps.
- Perform all incubation and wash steps under gentle rocking or rotation.

- Cover the incubation chamber with adhesive film during incubation, particularly when incubation is more than 2 hours or  $<70 \mu\text{l}$  of sample or reagent is used.
- Several incubation steps such as step 6 (blocking), step 7 (sample incubation), step 10 (detection antibody incubation), or step 13 (Cy3 equivalent dye-streptavidin incubation) may be done overnight at  $4^{\circ}\text{C}$ . Please make sure to cover the incubation chamber tightly to prevent evaporation.

## VIII. Protocol

---

**Note:** This product contains sets of reagents for different arrays. Always ensure you are using the proper glass slide, lyophilized standard mix, and biotinylated antibody cocktail for the correct corresponding array.

The following procedure is for processing any one of the arrays in the kit.


### A. Completely Air Dry The Glass Slide

1. Take out the glass slide from the box, and let it equilibrate to room temperature inside the sealed plastic bag for 20-30 minutes. Remove slide from the plastic bag, peel off the cover film, and let it air dry for another 1-2 hours.

*Incomplete drying of slides before use may cause the formation of "comet tails," thin directional smearing of antibody spots.*

### B. Prepare Cytokine Standard Dilutions

There is only one vial of standard provided in the two-slide kit, which is enough for making two standard curves. Reconstitute the lyophilized standard within one hour of usage. If you must use the standard for two different days, store only the Std1 dilution at  $-80^{\circ}\text{C}$ .

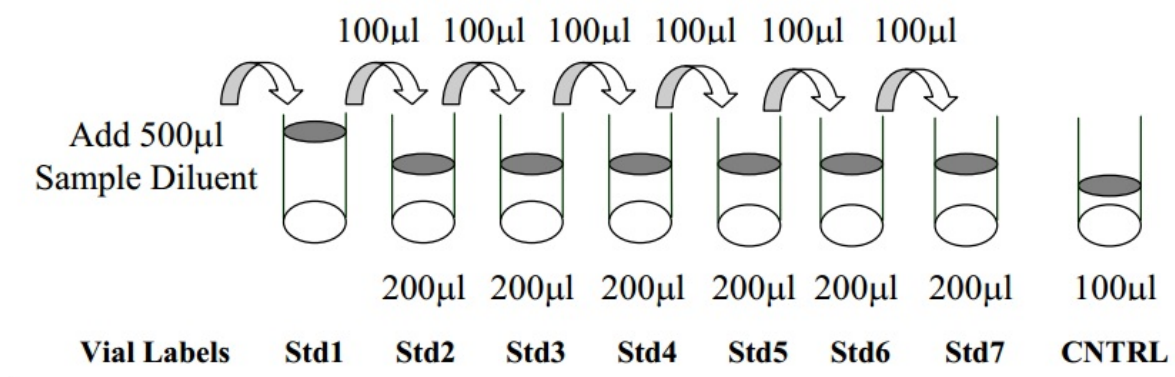



2. Reconstitute the Cytokine Standard Mix (lyophilized) by adding 500  $\mu$ l Sample Diluent to the tube. For best recovery, always quick-spin vial prior to opening. Dissolve the powder thoroughly by a gentle mix. Labeled the tube as Std1.
3. Label 6 clean microcentrifuge tubes as Std2 to Std7. Add 200  $\mu$ l Sample Diluent to each of the tubes.

4. Pipette 100  $\mu$ l Std1 into tube Std2 and mix gently. Perform 5 more serial dilutions by adding 100  $\mu$ l Std2 to tube Std3 and so on.
5. Add 100  $\mu$ l Sample Diluent to another tube labeled as CNTRL. Do not add standard cytokines or samples to the CNTRL tube, which will be used as negative control. For best results, include a set of standards in each slide.

*Since the starting concentration of each cytokine is different, the serial concentrations from Std1 to Std7 for each cytokine are varied which can be found in Section X.*

### **C. Blocking & Incubation**

6. Add 100  $\mu$ l Sample Diluent into each well and incubate at room temperature for 30 minutes to block slides.
7. Decant buffer from each well. Add 100  $\mu$ l standard cytokines or samples to each well. Incubate arrays at room temperature for 1-2 hour.

*Longer incubation time is preferable for higher signals. This step may be done overnight at 4°C.*

*We recommend using 50 to 100  $\mu$ l of original or diluted serum, plasma, conditioned media, or other body fluid, or 250  $\mu$ g/ml-1 mg/ml of protein for cell and tissue lysates. Cover the incubation chamber with adhesive film during incubation, especially if less than 70  $\mu$ l of sample or reagent is used.*

8. Wash:
  - Decant the samples from each well, and wash 5 times (5 min each) with 150  $\mu$ l of 1X Wash Buffer I at room temperature with gentle rocking. Completely remove wash buffer in each wash step. Dilute 20x Wash Buffer I with H<sub>2</sub>O.
  - *(Optional for Cell and Tissue Lysates)* Put the glass slide with frame into a box with 1X Wash Buffer I (cover the whole glass slide and frame with Wash Buffer I), and wash at room temperature with gentle rocking for 20 min.

- Decant the 1x Wash Buffer I from each well, wash 2 times (5 min each) with 150 µl of 1X Wash Buffer II at room temperature with gentle rocking. Completely remove wash buffer in each wash step. Dilute 20X Wash Buffer II with H<sub>2</sub>O.

*Incomplete removal of the wash buffer in each wash step may cause "dark spots," the background signals higher than the spots.*

#### **D. Incubation with Biotinylated Antibody Cocktail & Wash**

9. Reconstitute the detection antibody by adding 1.4 ml of Sample Diluent to the tube. Spin briefly.
10. Add 80 µl of the detection antibody cocktail to each well. Incubate at room temperature for 1-2 hour.

*Longer incubation time is preferable for higher signals and backgrounds*


11. Decant the samples from each well, and wash 5 times (5 mins each) with 150 µl of 1X Wash Buffer I and then 2 times with 150 µl of 1x Wash Buffer II at room temperature with gentle rocking. Completely remove wash buffer in each wash step.

#### **E. Incubation with Cy3 Equivalent Dye-Streptavidin & Wash**

12. After briefly spinning down, add 1.4 ml of Sample Diluent to Cy3 equivalent dye-conjugated streptavidin tube. Mix gently.
13. Add 80 µl of Cy3 equivalent dye-conjugated streptavidin to each well. Cover the device with aluminum foil to avoid exposure to light or incubate in dark room. Incubate at room temperature for 1 hour.
14. Decant the samples from each well, and wash 5 times (5 mins each) with 150 µl of 1X Wash Buffer I at room temperature with gentle rocking. Completely remove wash buffer in each wash step.

## F. Fluorescence Detection

15. Disassemble the device by pushing clips outward from the slide side. Carefully remove the slide from the gasket.

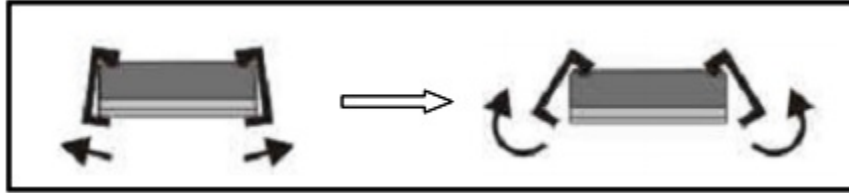

*Be careful not to touch the surface of the array side.*

16. Place the slide in the Slide Washer/Dryer (a 4-slide holder/centrifuge tube), add enough 1x Wash Buffer I (about 30 ml) to cover the whole slide, and then gently shake at room temperature for 15 minutes. Decant Wash Buffer I. Wash with 1x Wash Buffer II (about 30 ml) and gently shake at room temperature for 5 minutes.

17. Remove water droplets completely by gently applying suction with a pipette to remove water droplets. Do not touch the array, only the sides.

*You may also dry the glass slide by a compressed N<sub>2</sub> stream.*


18. Imaging: The signals can be visualized through use of a laser scanner equipped with a Cy3 wavelength (green channel) such as Axon GenePix, or Innopsys Innoscan. Make sure that the signal from the well containing the highest standard concentration (Std1) receives the highest possible reading, yet remains unsaturated.

*In case the signal intensity for different cytokine varies greatly in the same array, we recommend using multiple scans, with a higher PMT for low signal cytokines, and a low PMT for high signal cytokines.*

## G. Data Analysis

19. Data extraction can be done using the GAL file that is specific for this array along with the microarray analysis software (GenePix, ScanArray Express, ArrayVision, MicroVigene, etc.). GAL files can be found here: [www.RayBiotech.com/Gal-Files.html](http://www.RayBiotech.com/Gal-Files.html).

Need help analyzing all that data? Copy and paste your data into the Q-Analyzer Tool specific for this array, catalog number: **QAM-CAA-3000-SW**. More information can be found in Section XII.

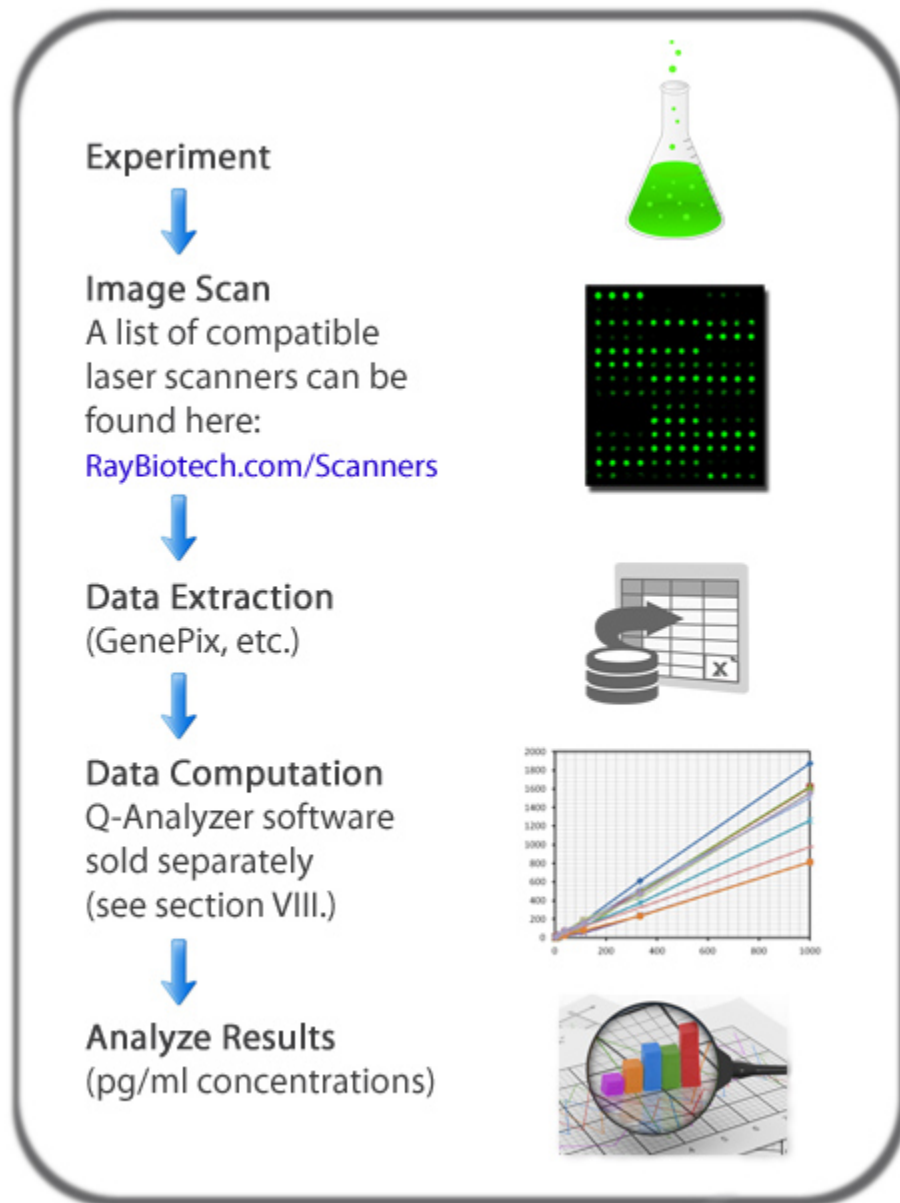

## IX. Array Map & Standard Curves

Please view the individual array manuals for representative standard curve images

QAM-CYT-4

Each antibody is printed in quadruplicate horizontally												
	1	2	3	4	1	2	3	4	1	2	3	4
A	POS1				POS2				Amphiregulin			
B	Axl				CD27 Ligand				CD30 (TNFRSF8)			
C	CD40 (TNFRSF5)				CXCL16				EGF			
D	E-Selectin				Fractalkine				GITR (TNFRSF18)			
E	HGF				IGFBP-2				IGFBP-3			
F	IGFBP-5				IGFBP-6				IGF-1			
G	IL-12 p70				IL-17E (IL-25)				IL-17F			
H	IL-1 ra (IL-1 F3)				IL-2 R alpha				IL-20			
I	IL-23 p19				IL-28A				I-TAC (CXCL11)			
J	MDC (CCL22)				MIP-2				MIP-3 alpha (CCL20)			
K	Osteopontin (SPP1)				Osteoprotegerin				Prolactin			
L	Pro-MMP-9				P-Selectin				Resistin			
M	SCF				SDF-1 alpha				Thrombopoietin (TPO)			
N	VCAM-1 (CD106)				VEGF-A				VEGF-D			

QAM-CYT-5

Each antibody is printed in quadruplicate horizontally												
	1	2	3	4	1	2	3	4	1	2	3	4
A	POS1				POS2				bFGF			
B	BLC (CXCL13)				CD30 Ligand				Eotaxin-1 (CCL11)			
C	Eotaxin-2 (MIPF-2)				Fas Ligand (TNFSF6)				GCSF			
D	GM-CSF				ICAM-1 (CD54)				IFN-gamma			
E	IL-1 alpha				IL-1 beta				IL-2			
F	IL-3				IL-4				IL-5			
G	IL-6				IL-7				IL-10			
H	IL-12 p40				IL-13				IL-15			
I	IL-17A				IL-21				KC (CXCL1)			
J	Leptin				LIX				MCP-1 (CCL2)			
K	MCP-5				M-CSF				MIG (CXCL9)			
L	MIP-1 alpha (CCL3)				MIP-1 gamma				Platelet Factor 4			
M	RANTES (CCL5)				TARC (CCL17)				I-309 (CCL1)			
N	TNF RI (TNFRSF1A)				TNF RII (TNFRSF1B)				TNF-alpha			

QAM-CYT-6

Each antibody is printed in quadruplicate horizontally												
	1	2	3	4	1	2	3	4	1	2	3	4
A	POS1				POS2				4-1BB (CD137)			
B	Ace				ALK-1				Cardiotriohin-1 (CT-1)			
C	CD27 (TNFRSF7)				CD40 Ligand				CTLA-4 (CD152)			
D	Decorin				DKK-1				Dtk			
E	Endoglin (CD105)				Fc-gamma-RIIB				Fit-3 Ligand			
F	Galectin-1				Galectin-3				Gas 1			
G	Gas 6				GITR Ligand				HAI-1			
H	HGFR				IL-1 R4 (ST2)				IL-3 R beta			
I	IL-9				JAM-A (CD321)				Leptin R			
J	L-selectin (CD62L)				Lymphotactin				MadCAM-1			
K	MFG-E8				MIP-3 beta (CCL19)				Neprilysin			
L	Pentraxin-3 (TSG-14)				RAGE				TACI			
M	TREM-1				TROY				TSLP			
N	TWEAK R				VEGF R1				VEGF R3			

QAM-CYT-7

Each antibody is printed in quadruplicate horizontally												
	1	2	3	4	1	2	3	4	1	2	3	4
A	POS1				POS2				CD80 (B7-1)			
B	BAFF R				Betacellulin (BTC)				C5a			
C	CCL6				CD48 (SLAMF2)				CD6			
D	Chemerin				Clusterin				CXCL15			
E	Cystatin C				DAN				DLL4			
F	EDAR				Endocan				Fetuin A			
G	H60				IL-33				IL-7 R alpha			
H	Kremen-1				Limitin				Lipocalin-2 (NGAL)			
I	LOX-1				Marapsin				MBL-2			
J	Meteorin				Nope				NOV (CCN3)			
K	Osteoactivin				OX40 Ligand				P-Cadherin			
L	Periostin				PIGF-2				Progranulin			
M	Prostasin				Renin 1				Testican 3			
N	TIM-1 (KIM-1)				TRAIL (TNFSF10)				Tryptase epsilon			

## **X. Standard Concentrations**

---

After reconstitution, the lyophilized cytokine standard mix contains the following concentrations for each antigen included.

QAM-CYT-4 (pg/ml)	QAM-CYT-5 (pg/ml)	QAM-CYT-6 (pg/ml)	QAM-CYT-7 (pg/ml)				
AR	2,000	bFGF	5,000	4-1BB	25,000	B7-1	4,000
Axl	10,000	BLC	10,000	ACE	100,000	BAFF R	1,000
CD27 L	20,000	CD30L	2,000	ALK-1	10,000	BTC	2,000
CD30 T	10,000	Eotaxin	1,000	CT-1	40,000	C5a	1,000
CD40	10,000	Eotaxin-2	1,000	CD27	25,000	CCL6	40,000
CXCL16	1,000	Fas L	10,000	CD40L	40,000	CD48	2,000
EGF	2,000	G-CSF	20,000	CTLA-4	2,500	CD6	1,000
E-Selectin	4,000	GM-CSF	10,000	Decorin	5,000	Chemerin	100,000
Fractalkine	100,000	ICAM-1	10,000	Dkk-1	40,000	Clusterin	100,000
GITR	4,000	IFNg	4,000	Dtk	20,000	CXCL15	200,000
HGF	20,000	IL-1a	2,000	Endoglin	10,000	Cystatin C	2,000
IGFBP-2	100,000	IL-1b	4,000	Fcg RIIB	10,000	DAN	100,000
IGFBP-3	20,000	IL-2	10,000	Flt-3L	25,000	DLL4	40,000
IGFBP-5	40,000	IL-3	2,000	Galectin-1	10,000	EDAR	20,000
IGFBP-6	40,000	IL-4	500	Galectin-3	2,000	Endocan	20,000
IGF-I	10,000	IL-5	10,000	Gas 1	2,000	Fetuin A	100,000
IL-12 p70	4,000	IL-6	4,000	Gas 6	2,500	H60	2,000
IL-17E	40,000	IL-7	10,000	GITR L	1,000	IL-33	4,000
IL-17F	40,000	IL-10	10,000	HAI-1	10,000	IL-7 R $\alpha$	40,000
IL-1ra	4,000	IL-12p40	1,000	HGF R	25,000	Kremen-1	4,000
IL-2 R $\alpha$	10,000	IL-13	20,000	IL-1 R4	40,000	Limitin	1,000
IL-20	20,000	IL-15	100,000	IL-3 Rb	40,000	Lipocalin-2	100,000
IL-23	40,000	IL-17	4,000	IL-9	20,000	LOX-1	4,000
IL-28	2,000	IL-21	20,000	JAM-A	5,000	Marapsin	20,000
I-TAC	20,000	KC	2,000	Leptin R	5,000	MBL-2	2,000
MDC	1,000	Leptin	100,000	L-Selectin	10,000	Meteorin	40,000
MIP2	1,000	LIX	20,000	Lymphotactin	200,000	Nope	10,000
MIP-3a	1,000	MCP-1	4,000	MadCAM-1	10,000	NOV	40,000
OPN	20,000	MCP-5	1,000	MFG-E8	40,000	Osteoactivin	10,000
OPG	20,000	M-CSF	2,000	MIP-3b	1,000	OX40 Ligand	4,000
Prolactin	10,000	MIG	10,000	Nepriylisin	20,000	P-Cadherin	4,000
Pro-MMP-9	100,000	MIP-1a	10,000	Pentraxin 3	10,000	Periostin	4,000
P-Selectin	4,000	MIP-1g	1,000	RAGE	25,000	PIGF-2	1,000
Resistin	2,000	PF-4	20,000	TACI	50,000	Progranulin	100,000
SCF	10,000	RANTES	4,000	TREM-1	10,000	Prostasin	100,000
SDF-1a	100,000	TARC	4,000	TROY	4,000	Renin 1	40,000
TPO	100,000	TCA-3	2,000	TSLP	4,000	Testican 3	40,000
VCAM-1	4,000	TNF RI	500	TWEAK R	25,000	TIM-1	100,000
VEGF	4,000	TNF RII	2,000	VEGF R1	10,000	TRAIL	10,000
VEGF-D	4,000	TNF $\alpha$	1,000	VEGF R3	10,000	Tryptase $\epsilon$	100,000



## **XI. Spiking & Recovery**

---

*Please view the individual array manuals for spiking & recovery data*

## XII. Quantibody<sup>®</sup> Q-Analyzer

---

The Q-Analyzer is an array specific, Excel-based program. It is much more than a simple calculation macro; it performs sophisticated data analysis (see below for description).

The Q-Analyzer Tool specific for this array is catalog number: **QAM-CAA-3000-SW**.

### Key features:

- Simplicity: Easy to operate and requires no professional training. With a simple copy and paste process, the cytokine concentration is determined.
- Outlier Marking & Removing: The software can automatically mark and remove the outlier spots for more accurate data analysis
- Normalization: The program allows for intra- and inter-slide normalization for large numbers of samples.
- Two Positive Controls: The program utilizes the two positive controls in each array for normalization.
- Two Analytical Algorithms: Users can choose either linear regression or log-log algorithms to meet their analytical needs.
- Two Data Outputs: standard curves and digital concentration.
- User Intervention: The program allows for user manual handling of outliers and other analytical data.
- Lower and Upper Limits Determination: The program automatically marks out the values below or above the detection range.
- Standard Deviation: The program outputs the standard deviations of the quadruplicate spots for data accuracy.
- Analytical Tips: Q-Analyzer analysis tips are included in the program.

### XIII. Troubleshooting Guide

<b>Problem</b>	<b>Cause</b>	<b>Recommendation</b>
<b>Weak Signal</b>	Inadequate detection	Increase laser power and PMT parameters
	Inadequate reagent volumes or improper dilution	Check pipettes and ensure correct preparation
	Short incubation time	Increase incubation time or change sample incubation step to overnight
	Too low protein concentration in sample	Lessen dilution or do not dilute sample. Concentrate sample if necessary.
	Improper storage of kit	Store kit as suggested temperature. Don't freeze/thaw the slide.
<b>Uneven signal</b>	Bubble formed during incubation	Decrease amount of rocking during incubations. check for bubble formation and remove bubbles.
	Arrays are not completely covered by reagent	Completely cover arrays with solution for all required steps.
	Reagent evaporation	Cover the incubation chamber with adhesive film during incubation
<b>Poor standard curve</b>	Cross-contamination from neighboring wells	Avoid overflowing wash buffer and other solutions into neighboring wells.
	Comet tail formation	Air dry the slide for at least 1 hour before usage
	Inadequate standard reconstitution or Improper dilution	Reconstitute the lyophilized standard well at the room temperature before making serial dilutions. Check pipettes and ensure proper serial dilutions.
	Inadequate detection	Increase laser power so the highest standard concentration for each cytokine receives the highest possible reading yet remains unsaturated.
	Use freeze-thawed cytokine standards	Always use new cytokine standard vial for new set of experiment. Discard any leftover.
<b>High background</b>	Overexposure	Lower the PMT or signal gain.
	Dark spots	Completely remove wash buffer in each wash step.
	Insufficient wash	Increase wash time and use more wash buffer
	Dust	Work in clean environment
	Slide is allowed to dry out	Don't dry out slides during experiment.

## XIV. Select Quantibody<sup>®</sup> Publications

---

1. Zeng Q., et al. The functional behavior of a macrophage/fibroblast co-culture model derived from normal and diabetic mice with a marine gelatin-oxidized alginate hydrogel. *Biomaterials*. 2010 Aug;31(22):5772-81. doi: 10.1016/j.biomaterials.2010.04.022.  
**Species:** Mouse
2. Toh H, Wang W, Chia W, Kvistborg P, Sun Li, et al. Clinical Benefit of Allogeneic Melanoma Cell Lysate-Pulsed Autologous Dendritic Cell Vaccine in MAGE-Positive Colorectal Cancer Patients. *Clin Cancer Res*. 2009;15(24):7726-7736  
**Species:** Human  
**Sample Type:** Plasma
3. Du Y, Wei X, He Y, Wei G, Hampel H, et al. P2-380: Identification and characterization of human autoantibodies that may be used for the treatment of prion diseases. *Alzheimer Dementia*. 2008;4(4 Suppl):T484 (Abstract P2-380).  
**Species:** Human  
**Sample Type:** Plasma
4. Jonnalagadda D., et al. Platelet secretion is kinetically heterogeneous in an agonist-responsive manner. December 20, 2012; *Blood*: 120 (26). <http://dx.doi.org/10.1182/blood-2012-07-445080>  
**Species:** Human  
**Sample Type:** Conditioned Media
5. Vargas-Inchaustegui D., Hogg A., Tulliano G., et al. CXCL10 Production by Human Monocytes in Response to *Leishmania braziliensis* Infection. *Infect. Immun*. January 2010 vol. 78 no. 1 301-308  
**Species:** Human  
**Sample Type:** Serum
6. Zhai Y, Zhong Z, Chen C-YA, Xia Z, Song L, Blackburn MR, Shyu A-B. Coordinated Changes in mRNA Turnover, Translation, and RNA Processing Bodies in Bronchial Epithelial Cells following Inflammatory Stimulation. *Mol Cell Biol*. 2008; 28(24):7414-7426.  
**Species:** Human
7. Huggenberger R., et al. Stimulation of lymphangiogenesis via VEGFR-3 inhibits chronic skin inflammation. *J Exp Med*. 2010 Sep 27;207(10):2255-69. doi: 10.1084/jem.20100559.  
**Species:** Mouse  
**Sample Type:** Tissue Lysate
8. Jurk D., Wilson C., Passos J., et al. Chronic inflammation induces telomere dysfunction and accelerates ageing in mice. *Nature Communications* 2, Article number: 4172. doi:10.1038/ncomms5172  
**Species:** Mouse  
**Sample Type:** Conditioned Media
9. Bethunaickan, R., Sahu, R., Liu, Z., Tang, Y. T., Huang, W., Edegbe, O., Tao, H., Ramanujam, M., Madaio, M. P. and Davidson, A. (2012), Anti-tumor necrosis factor alpha treatment of interferon-alpha-induced murine lupus nephritis reduces the renal macrophage response but does not alter glomerular immune complex formation. *Arthritis & Rheumatism*, 64: 3399-3408. doi: 10.1002/art.34553  
**Species:** Mouse  
**Sample Type:** Tissue Lysate
10. Hou T., Li Z., Luo F., Xie Z., Wu X., Xing J., Dong S., Xu J. A composite demineralized bone matrix e Self assembling peptide scaffold for enhancing cell and growth factor activity in bone marrow. *Biomaterials*, Available online 19 April 2014. [Epub ahead of print]  
**Species:** Mouse  
**Sample Type:** Tissue Lysate
11. Feng W., Madajka M., Kerr B., Mahabeleshwar G., White S., Byzova T. A novel role for platelet secretion in angiogenesis: mediating bone marrow-derived cell mobilization and homing. *Blood* April 7, 2011 vol. 117 no. 14 3893-3902  
**Species:** Mouse

# XV. Experiment Record Form

---

Date: \_\_\_\_\_

File Name: \_\_\_\_\_

Laser Power: \_\_\_\_\_

PMT: \_\_\_\_\_

Well No.	Sample Name	Dilution factor
1	CNTRL	
2	Std7	
3	Std6	
4	Std5	
5	Std4	
6	Std3	
7	Std2	
8	Std1	
9		
10		
11		
12		
13		
14		
15		
16		

1	2
3	4
5	6
7	8
9	10
11	12
13	14
15	16

## XVI. How to Choose a Quantibody<sup>®</sup> Array?

---

### Species-based selection:

Human (QAH-)	Mouse (QAM-)	Rat (QAR-)	Bovine (QAB-)	Canine (QAC-)
Equine (QAE-)	Feline (QAF-)	Primates (QAN-)	Porcine (QAP-)	Rabbit (QAL-)

### Function-based selection:

Adhesion Molecule Arrays	Angiogenesis Arrays	Bone Metabolism Arrays	Chemokine Arrays
<b>Custom Arrays</b>	Cytokine Arrays	Growth Factor Arrays	IGF Signaling Arrays
IL-1 Family Arrays	Immune Response Arrays	Inflammation Arrays	Interleukin Arrays
Isotyping Arrays	MMP Arrays	Obesity Arrays	Ophthalmic Arrays
Periodontal Disease Arrays	Receptor Arrays	Th1/Th2/Th17 Arrays	

### Cytokine Number-based selection:

Arrays are available in the Quantibody<sup>®</sup> platform to detect 1000 human, 200 mouse, or 67 rat proteins. GLP-Compliant testing services are also available.

---

To learn more about the Quantibody<sup>®</sup> Antibody Array, visit [www.RayBiotech.com/Quantibody-Multiplex-Elisa-Array.html](http://www.RayBiotech.com/Quantibody-Multiplex-Elisa-Array.html)

Quantibody<sup>®</sup> is the trademark of RayBiotech, Inc.  
This product is for research use only.



©2015 RayBiotech, Inc